

# WINDAQ Acquisition Waveform Recording Software

WINDAQ Waveform Browser

Playback and Analysis Software

# ActiveX Controls and XControls

User's Manual Manual Revision M

Copyright © 2015 by DATAQ Instruments, Inc. The Information contained herein is the exclusive property of DATAQ Instruments, Inc., except as otherwise indicated and shall not be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any human or computer language, in any form or by any means, electronic, mechanical, magnetic, optical, chemical, manual, or otherwise without expressed written authorization from the company. The distribution of this material outside the company may occur only as authorized by the company in writing.

DATAQ Instruments' hardware and software products are not designed to be used in the diagnosis and treatment of humans, nor are they to be used as critical components in any life-support systems whose failure to perform can reasonably be expected to cause significant injury to humans.

DATAQ, the DATAQ logo, and WINDAQ are registered trademarks of DATAQ Instruments, Inc. All rights reserved.



241 Springside Dr. Akron, Ohio 44333 U.S.A. Telephone: 330-668-1444 Fax: 330-666-5434 Designed and manufactured in the United States of America

# Software License Agreement

### NOTE

DATAQ Instruments' hardware and software products are NOT designed to be used in the diagnosis and treatment of humans, nor are they to be used as critical components in any life-support systems whose failure to perform can reasonably be expected to cause significant injury to humans.

# LICENSE AGREEMENT

#### (SINGLE-USER PRODUCTS)

THIS IS A LICENSE AGREEMENT AND NOT AN AGREEMENT FOR SALE. A LICENSE AGREEMENT IS A LEGAL AGREEMENT BETWEEN YOU, THE END USER, AND DATAQ INSTRUMENTS, INC. PLEASE READ THIS LICENSE AGREEMENT CAREFULLY BEFORE OPENING THIS SEALED PACKAGE, OR ACCEPTING ITS TERMS ELECTRONICALLY. IF YOU DO NOT AGREE WITH THE TERMS AND CONDI-TIONS OF THIS LICENSE AGREEMENT, PROMPTLY RETURN THE PACKAGE UNOPENED AND YOUR MONEY WILL BE REFUNDED, OR IF DELIVERED ELECTRONICALLY PRESS THE "DO NOT ACCEPT AND STOP" BUTTON.

#### 1. This software package is protected by federal copyright law and international treaty.

2. By law, you, the end user, may do the following: a) make a copy of the software solely for backup or archival purposes, or other copies only in accordance with item (4) below.

3. Federal copyright law prohibits you from making any other copy of the software for any other reason without our permission. Federal copyright law also prohibits you from copying the written materials accompanying the software without first obtaining our permission.

4. You may install our WinDaq data acquisition software on multiple computers, provided that one software license has been purchased (or granted) for each DATAQ Instruments hardware unit that is to be used with the software. For example, the purchase of one hardware unit and one software unit allows you to install the software on as many computers as desired. But if a second unit is purchased, that unit cannot be used with the original license installed on any computer unless a second license is also purchased. To do otherwise is a violation of this License Agreement. This restriction does not include licenses for WinDaq Waveform Browser (playback) software, which are free.

5. If the software is a library product, then you have a royalty-free right to reproduce executable files created using the software.

6. You may not alter, modify or adapt the software or accompanying materials. In addition, you may not translate, decompile, disassemble or reverse engineer the software. You also may not create any derivative works based on this software. A derivative work is defined as a translation or other form in which the software may be recast, transformed or adapted.

### **LIMITED WARRANTY**

DATAQ Instruments, Inc. warrants that this program will perform in substantial compliance with the published specifications and documentation supplied in this package, provided it is used on the computer hardware and with the operating system for which it was designed. This warranty is limited to a period of 90 days from the date of the original purchase.

If you report a significant defect in performance, in writing within 90 days of purchase, DATAQ Instruments will attempt to correct it or, at its option, authorize a refund of your license fee.

DATAQ Instruments warrants that the original disks and documentation are free from defects in material and workmanship, assuming normal use, for a period of 90 days from the date of purchase. If a defect occurs during this period, you may return the faulty disk or documentation, along with a dated proof of purchase, and DATAQ Instruments will replace it free of charge. Except as specifically provided above, DATAQ Instruments makes no other warranty or representation, either express or implied, with respect to this software, the disks or documentation, including their quality, merchantability, or fitness for a particular purpose. In no event will DATAQ Instruments be liable for direct, indirect, special, incidental, or consequential damages arising out of the use or inability to use the software or documentation, even if DATAQ Instruments has been advised of the possibility of such damages. The warranties and remedies set forth above are exclusive and in lieu of all others, oral or written, express or implied.

DATAQ Instruments is not responsible for any costs including, but not limited to, those incurred as a result of lost profits or revenue, loss of time or use of the software, loss of data, the costs of recovering such software or data, the cost of substitute software, claims by third parties, of other similar costs. In no case will DATAQ Instruments' liability exceed the amount of the license fee. The warranties provided give you specific legal rights. You may have other rights which vary from state to state. Some states do not allow the exclusion of incidental or consequential damages, or the limitation of how long an implied warranty lasts, so some of the above may not apply to you.

DATAQ Instruments retains title to and ownership of the software. DATAQ Instruments retains all rights not expressly granted. Nothing in this License Agreement constitutes a waiver of DATAQ Instruments' rights under the U.S. copyright laws or any other Federal or State law. DATAQ Instruments or its designee has the right to audit your computer and software usage to determine whether any unauthorized copies of this program have been made. Any authorized copy of the software covered by this Agreement, including authorized backup copies if any, must include DATAQ Instruments' copyright and trademark notices.

#### **U.S. GOVERNMENT RESTRICTED RIGHTS**

The software covered by this Agreement and documentation thereto are provided with RESTRICTED RIGHTS. Use, duplication or disclosure by the Government is subject to restrictions as set forth in subparagraph (c)(l)(ii) of the Rights in Technical Data and Computer Software clause at 52.227-7013. The manufacturer of this software and documentation thereto is DATAQ Instruments, Inc.; 241 Springside Drive; Akron, Ohio 44333; (330) 668-1444.

This Agreement is governed by the State of Ohio in the United States of America.

If you have any questions about this License Agreement, write to: DATAQ Instruments, Inc.; 241 Springside Drive; Akron, Ohio 44333.

# Table of Contents

	ftware License Agreement ble of Contents	
	Introduction	
1.	WinDag Software	
	Help Files	
	Multimedia Demonstration Videos	
	Conventions Used in the Documentation	
	General Conventions	
	Mouse Conventions	
2	WinDaq Operating Modes	. 5
2.	Getting Started	. 3
5.	Help Files	. 7
	Fast Start	
	Step 1 Enabling Channels for Acquisition	
	DI-145 USB Data Acquisition Starter Kit	· 7
	All Other DATAQ Instruments Product	. /
	Enabling/disabling a channel	. 0
	Enabling/disabling a differential channel	
	Enabling a digital input channel	. 9
	Channel Selection Notes	. 10
	Step 2 Viewing Enabled Channels	
	Step 3 Specifying a Sample Rate	. 12
	DI-149 USB Data Acquisition Starter Kit	. 12
	All Other Products	
	WinDaq/Pro+	
	Step 4 Specifying Gain and Measurement Range	. 14
	Step 5 Converting Volts to Engineering Units	. 13
	Step 6 Recording Waveforms to Disk	. 1/
	Event Markers	. 20
	Triggered Sweep Display	
	Triggered Mode (as supported by your bardware)	20
	Triggered Mode (as supported by your hardware) Reference Files	20
	User Annotation	$\frac{20}{20}$
4	WinDaq Waveform Browser	
	Help Files	21
	Fast Start	
	Step 1 Moving Around in the Data File	21
	Moving Coarsely Through the Data File with the Scroll Bar	21
	Moving to a Single Point Using the Cursor	
	Step 2 Time and Date Display	. 22
	Start Time	. 22
	End Time	. 23
	Cursor Time	
	Time/Division	
	Step 3 Making Waveform Measurements with the Cursor	
	Selecting a Channel	. 23
	The Data Cursor	. 23
	Moving the Cursor to the highest peak	
	Moving the Cursor to the lowest valley	. 24
	Moving the Cursor to the Center of the Screen	. 25
	Step 4 Getting a Bird's Eye View of All the Data or a Portion of the Data	. 25

Compressing all Data	25
Compressing to a Ratio	
Cursor Mode Control (Mid/Min/Max/MxMn) for compressed displays	25
Step 5 Making Statistics Measurements	
Step 6 Exporting to Excel	27
Additional Playback Features	$\overline{32}$
X-Y plotting	
FFT and DFT utilities	32
Event Markers	
5. ActiveX Controls	
Help Files	
Accessing ActiveX Controls	
DataqFile	
ŴriteDataqFile	34
ReadDataqFile	
DataqSDK	
DataqSerial (Obsolete)	35
DQChart	
WinDag	
6. XControls Software Option	37
Installing XControl Software	37
Using XControls with WinDaq/XL	37
Step One:	38
Step Two:	
Step Three:	
Step Four:	41
XControls Documentation	41
Index	43

# 1. Introduction

This manual contains information designed to familiarize you with and provide a "Fast Start" for WINDAQ waveform recording software, WINDAQ Waveform Browser playback and analysis software, ActiveX Controls, and XControls Software Option. For a complete and detailed description of each function contained in WINDAQ software please use the Help Files.

# WINDAQ Software


Use WINDAQ software with any DATAQ Instruments hardware product. The WINDAQ software package contains both recording and playback software. The recording software allows you to record waveforms directly and continuously to disk while monitoring a real time display of the waveforms on your computer screen.

**WINDAQ/Lite** Recording Software limits maximum throughput to 240 Hz when in RECORD mode. **WINDAQ/Pro** Recording Software features a sample rate limited only by the maximum sample rate of the hardware. In addition to WINDAQ/Pro's features, **WINDAQ/Pro+** Recording Software allows you to tailor sample different channels at different rates by entering a sample rate divisor value (1 to 255) for each channel.


**WINDAQ Waveform Browser** playback software allows you to review, measure, analyze, compress, cut-and-paste, export/import, and otherwise manipulate the recorded waveform information.

## Help Files

Click an item in the **Help** menu or use the context-sensitive help feature encoded into the software to access the Help Files. The Help menu provides links to specific Help Topics. For example, clicking on **Mouse** in the **Help** menu will take you to the portion of the help file regarding Mouse operations. Highlight a menu item and press **F1** to utilize the **context-sensitive help** feature. The Help File will open to the page most relevant to that menu item, its functionality, and activating procedure.

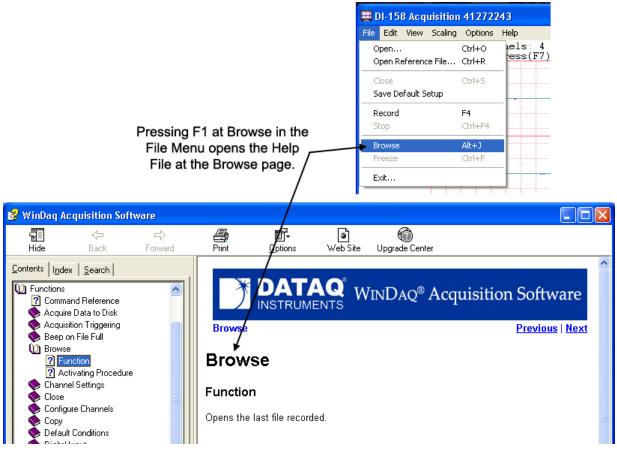

Help Files contain 3 basic window panes. The **Options** pane gives printing options, browser functionality, and some helpful links to our web site. The **Contents** pane has three tabs - the Contents, Index, and Search Tabs. These tabs provide an easy way to find exactly the help information you need. The **Main** pane shows the main text and also provides browsing functionality to the help file. Click on the Next and Previous links to browse through the Help File comparable to paging through a book.

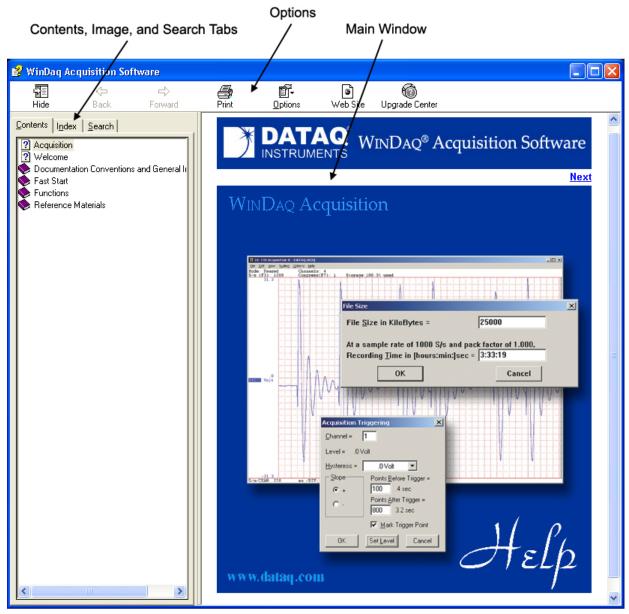

# Multimedia Demonstration Videos

The icon shown below indicates the availability of a Multimedia Demonstration Video on the internet via YouTube or in the help files for that particular subject. Click on the icon to view the Demo (**internet connection required**) or open the Help Files to view any of the WINDAQ Software Demonstration Videos.



# Conventions Used in the Documentation

Before using WINDAQ software, please read this section to understand some of the terms and notational conventions used here and in the Help Files.

# **General Conventions**

Commands you choose are given with the menu name preceding the command name. For example, the phrase "Choose File Open" tells you to choose the Open command from the File menu. This naming convention describes the sequence you follow in choosing a command - first you select the menu, then you choose the command.

# **Mouse Conventions**

In general, most mouse actions require only the left mouse button. For example, carrying out a menu command or working in a dialog box requires only the left mouse button. Since the majority of mouse procedures are done with the left mouse button, we will not specify which mouse button to click, drag, or double-click in the procedure unless the action uses the RIGHT mouse button. For example, "Double-click the right mouse button anywhere in the bottom annotation line to move the cursor to the lowest displayed waveform valley."

- "Point" means to position the mouse pointer until the tip of the pointer rests on what you want to point to on the screen. For example, "Point to the View menu."
- "Click" means to press and immediately release the mouse button without moving the mouse. For example, "To display the menu that contains the command you want, click the menu name in the menu bar."
- "Double-click" means to click the mouse button twice in rapid succession. For example, "Double-click the icon to start the program."
- "Drag" means to press the mouse button and hold it down while you move the mouse; then release the button. For example, "Drag down to Data Cursor to enabled the cursor for on-screen display."

# WINDAQ Operating Modes

WINDAQ waveform recording software has three operating modes: Setup, Record, and Standby. Each operating mode shares many features with the other two, but specific modes may restrict features or disable some functions altogether.

WINDAQ Recording Software starts in the SET UP operating mode. In SET UP mode you can configure data acquisition parameters—such as the number of acquired channels, channel gain, and channel offset—and customize the real time display. SET UP operating mode provides access to most data acquisition functions and adjustments including control of the real time display screen's scaling and offset functions. The SET UP mode displays data in real time but does not store data to disk. This mode limits sample rate only by the capabilities of the hardware. In other words, you can sample as fast as your instrument will allow. When in this mode, the Status: area of the bottom annotation line displays SET-UP.

The RECORD operating mode stores, or streams, data to disk. Activate the RECORD mode by selecting Record from the File menu. You can use all waveform recording features and functions (with some restrictions) while in the RECORD mode except the following: Channel-specific operations (i.e., channel number, gain, offset) and sample rate adjustments. Waveform information continuously streams to disk while the real time display remains active. RECORD mode limits sample rate to 240 Hz maximum throughput when using WINDAQ/Lite but does not limit the sample rate when using WINDAQ/Pro or Pro+ (limit determined by hardware). When in RECORD mode, the Status: area of the bottom annotation line displays RECORD.

Use the STANDBY operating mode to temporarily suspend (pause) waveform recording to disk. Select Stop in the File menu to enter STANDBY mode. You can use all waveform recording features and functions except channel-specific operations (i.e., channel number, offset, etc.) and sample rate adjustments. The STANDBY mode displays data in real time while waveform recording to disk has been stopped. When in this mode, the Status: area of the bottom annotation line displays STBY. Start and stop as many times as desired during a data acquisition session.

# 2. Getting Started

The following items are included with each instrument purchase. Verify that you have the following:

- Your DATAQ Instruments, Inc. hardware device.
- Appropriate communications cables (this will vary according to the instrument you purchased).
- The DATAQ Instruments Resource CD-ROM (if provided some devices do not come with a CD).
- This user's manual, which documents WINDAQ Software.

Call DATAQ Instruments at 330-668-1444 to report missing or damaged items—we will guide you through the appropriate steps for replacing them. Save the original packing material in the unlikely event that your unit must, for any reason, be sent back to DATAQ Instruments, Inc.

Refer to your hardware documentation for hardware and software installation instructions. Once installed, connect input signals as described in your hardware manual.

Once everything is installed and connected start WinDaq Acquisition software. A real-time display of signals displays on your screen.

# 3. WINDAQ Data Acquisition

WINDAQ Data Acquisition Software acquires, displays, and records waveform data. Before running the software, you must correctly install all hardware and software components and connect your signals. Follow the basic steps presented in this chapter for a fast start to your first data acquisition session. These fast start steps outline the condensed procedure for recording waveforms to disk. You will perform most of these functions every time you record with WINDAQ Acquisition.

# Help Files

For a complete description of all software functions, see the context-sensitive Help Files. To access the context sensitive help either highlight a menu item and press F1 (this will take you directly to help regarding that menu item) or go to the **Help** menu and click on **Contents**. The Help Files elaborate and detail the functions in this Chapter and contain detailed descriptions of each additional function available in WINDAQ Acquisition Software. After you have become familiar with the functions described here, take some time to look over the rest of the functions detailed in the Help Files.

# Fast Start

# Step 1 Enabling Channels for Acquisition

# **DI-145 USB Data Acquisition Starter Kit**

1. In the Edit menu click on Channels....



The Ch: block cursor will blink in the Channels field on the status bar. The currently active list of enabled channels are displayed in this field, immediately to the left of the cursor (blinking prompt).

	01-14	ō Acq	uisition							
Eile	<u>E</u> dit	⊻iew	Scaling	Options	Help					
Mode S∕s		scil) ): 24			nnels press	: 1,2,3, (F7): 1	<b>4</b> )	h: Storage:		% used
	10	000	: :	: :			1		_	
				cu	urrent	ly active		bli	nkin	g prompt
					char	mels				

- 2. Enter the desired channel number and press the ENTER key. Repeat for each desired channel. Each activated channel will have its corresponding channel number displayed in the currently active channels list.
- 3. When all desired channels have been enabled, exit the channel configuration routine by pressing any key other than the "D" or "I" key.


Type the channel number preceded by a minus ("-") sign to disable channels. For example, typing "-3" disables channel 3 and removes it from the list of currently active channels.

Note: You may not enable channels in RECORD mode.

### All Other DATAQ Instruments Product


You may enable or configure channels for acquisition only in SET-UP mode—you cannot add, delete, or configure channels in RECORD mode. To activate ADC channel configuration click on Channels... in the Edit Menu or double-click on the Channels: field in the status bar. This displays the Channel Selection grid.



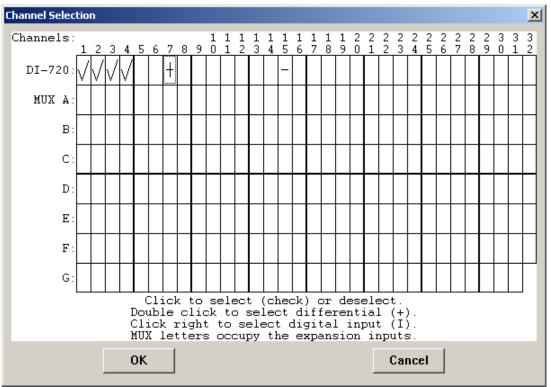

The channel selection grid displays the current status of all channels and allows you to enable and disable channels. In the illustration above, the boxes formed by the top row of the grid represent the internal channels available on the hardware device (the numbers above the top row of boxes refer to the channel numbers). The above example shows a DI-720 with channels 1-4 configured for single-ended inputs and channel 7 configured for differential input. The subsequent rows underneath the top row of the grid (labeled A, B, C, etc.) represent each group of 32 external analog input channels activated through use of an analog channel expander (like a DI-725).

The next graphic displays a single DI-725 32-channel analog expander added to the original DI-720. Enable and disable channels for an analog channel expander in Row A. At the end of the row labeled DI-720, you'll notice a pair of "A"s in the 31 and 32 positions. This indicates active status for the DI-725 and successful communication with the DI-720. WINDAQ Acquisition reserves channels 31 and 32 of the DI-720 to multiplex with the DI-725 (these channels cannot receive direct input when multiplexed). Channel 31 multiplexes the first 16 channels on the attached channel expander and channel 32 multiplexes the next 16 channels. Adding a second expander displays a "B" at channels 29 and 30 indicating use by the second expander. Each expander added continually increments channels in this manner.

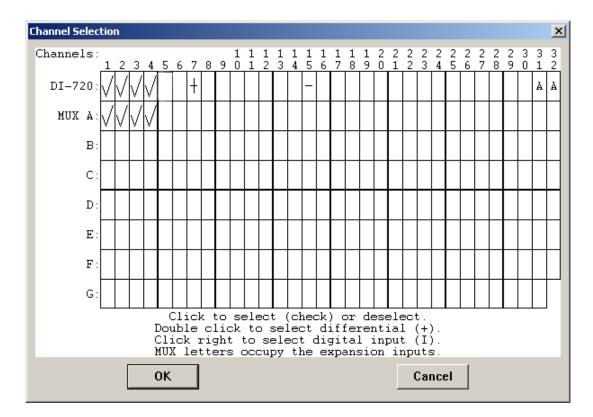

Use the instructions below to enable a channel for single-ended, differential, or digital input.

#### Enabling/disabling a channel

A check mark in the channel box indicates an enabled channel. Click on a channel box to enable/disable a channel and place/remove a check mark in/from its channel box.

#### Enabling/disabling a differential channel

**Note:** If your instrument has fixed differential channels (like models DI-722-16, DI-722-32, DI-730) enable the channels as noted above—place a check mark in the desired channel box. If your instrument does not have fixed differential channels, follow these procedures to designate channels as differential. See your hardware manual to determine if your instrument has fixed differential channels or not.


Point to the box in the grid representing the desired channel and double-click the left mouse button. This will display a plus sign (+) in the desired channel box. Double-clicking a second time removes the plus sign and disables the channel.

*Note:* You cannot enable a differential channel numbered higher than one half the total number of channels provided by the device (assuming the device supports differential inputs).

A differential channel requires two input terminals (positive and negative). For example, in order to designate channel 1 as differential requires both the channel 1 input terminal (positive input) and the channel 9 input terminal (negative input). Enabling a differential channel automatically enables its corresponding input (the negative terminal) and places a minus sign (-) in the Channel Selection grid, designating it as the low input of the differential pair.

#### Enabling a digital input channel

An "I" in the channel box indicates a digital channel. Right-click on a channel box to enable/disable a channel and place/remove an "I" in/from its channel box.

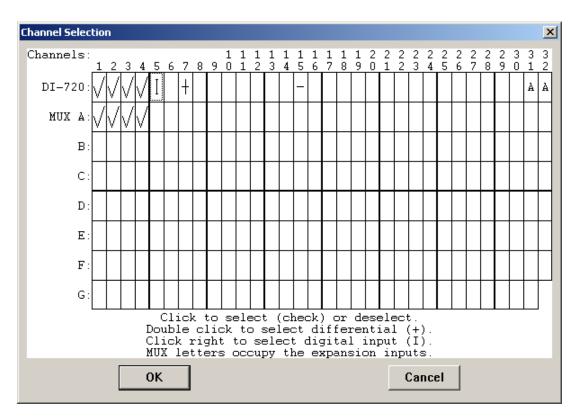

WINDAQ Acquisition acquires the eight digital input bits (accessible as defined by the hardware) on a digital input channel and scales the acquired data between +128 and -128, with 0 in the center.

Selecting **Digital Plot** in the **Scaling** menu will also display digital data. This feature horizontally splits the waveform strip configured for digital input into eight equal parts. WINDAQ assigns the top-most waveform as digital input 0, the bottom-most digital input 7, with the remaining 6 digital inputs allocated in logical order within the strip. This feature provides quick-look capability to determine the state of a digital input line.

### **Channel Selection Notes**

Single-ended, differential, and digital channels may coexist in any combination that the hardware allows.

WINDAQ Acquisition always sequentially samples from the lowest channel number specified to the highest.


You may enable any number and any combination of channels that the hardware will allow.

The RECORD mode does not allow configuration of the number or type of channels enabled.

## Step 2 Viewing Enabled Channels


The default number of channels displayed varies by instrument. Click on **Format Screen** in the **View** menu to change the current display. In the format box, click the desired display format. **Format Screen** allows for overlapped and non-overlapped waveform displays.



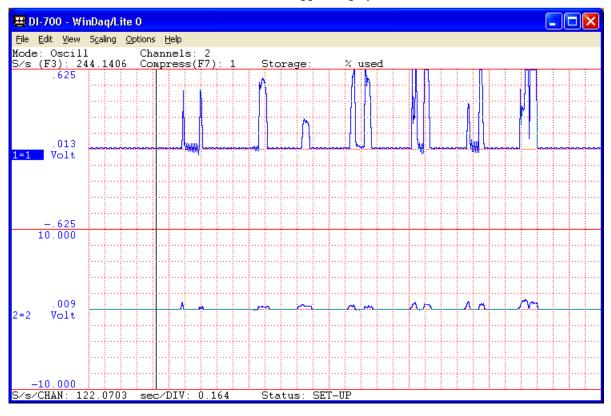

non-overlapped display

#### overlapped display

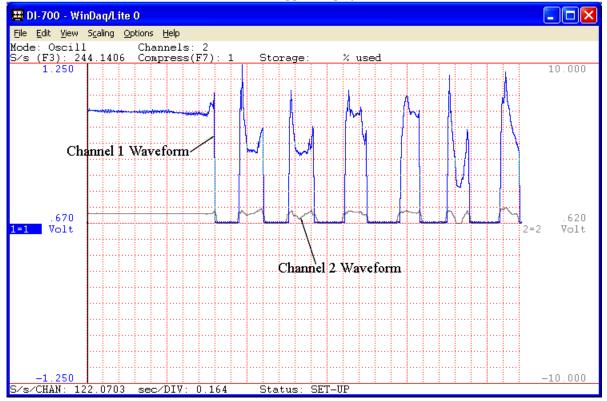

WINDAQ Acquisition 11

An overlapped format allows you to closely examine the relationship between two waveforms. A non-overlapped format allows you to isolate each waveform's transition to within a defined area. Whatever the timing relationship of your input signals, use any display format at any time without affecting the waveform information stored to disk. Display format changes only affect the way you view waveforms on your computer's monitor.

*Note:* To display eleven channels (or some other number not listed in *Format Screen*) select the User-specified option and enter 11 in the Number of Channels dialog box.

# Step 3 Specifying a Sample Rate

The total sample throughput rate is the rate that your instrument acquires samples for all channels combined. For example, to acquire two channels of data at 100Hz each would require a sample throughput rate (total scanning rate) of 200Hz (2 channels  $\times$  100Hz = 200Hz). The Sample Rate must be specified before recording; default varies.

😐 DI-154 Acquisition			
<u>File E</u> dit <u>V</u> iew S <u>c</u> aling	Options <u>H</u> elp		
Mode: Oscill S/s (F3): 240	Channels: 1,2,3,4 Compress(F7): 1	Storage:	% used
	· · · · · · · · ·	· · · · ·	

current sample rate

### **DI-149 USB Data Acquisition Starter Kit**


Specify a *per channel* sample rate:

1 In the Edit menu click on Sample Rate.... This displays the sample rate dialog box:

Sample Rate	
Channels enabled = 8	
Total Sample Rate = 2	40
Set Maximum rate/chan	nel = 30
Set Minimum rate/chan	nel = .0009156
Sample Rate/Channel = 🛛	30
ОК	Cancel

- 2. Enter the desired sample rate per channel in samples per second in the **Sample Rate/Channel** text box. Click on a **Set** button to have WinDaq automatically set your per channel sample rate to the maximum or minimum allowed for your throughput rate. *Please Note:* WinDaq/Lite will display a total sample throughput rate of 10,000 Hz (or 1250 Hz per channel) but will not record at rates over 240 Hz throughput (30 Hz per channel). You must purchase WinDaq/HS to record at rates over 240 Hz throughput.
- 3. Click **OK** or press the **ENTER** key.

The sample rate per channel is displayed in the lower left corner of the window as S/s/CHAN: (samples per second per channel).



### All Other Products

Specify a *throughput* rate:

1. In the Edit menu click on Sample Rate... . This displays the sample rate dialog box.




Samp	e Rate		×
Input	Buffer Size in Kilol	Bytes = 0	
Disk	Buffer Size in KiloE	Bytes = 64	
Sam	ple Rate =	240	
	ОК	Cancel	

- 2. Enter the desired data throughput rate (or total scanning rate) in samples per second in the **Sample Rate** dialog box.
- 3. Click **OK** or press the **ENTER** key.

WINDAQ Acquisition automatically allocates the correct amount of buffer space needed for the sample rate specified. The Input Buffer Size and Disk Buffer Size values display for informational purposes only.

Keep in mind that sample rate equals throughput rate. The current sample rate per channel (obtained by dividing the selected sample throughput rate by the number of channels enabled) displays in the lower left corner of the window as S/s/CHAN: (samples per second per channel).



sample rate per channel

You may specify/configure any sample rate that the hardware/software allows but you might not achieve the specific rate desired. For example (due to the inability to divide the master clock in a manner that results in an even-numbered quotient), you may see a sample rate of 2999.63 when you entered 3000.


### WINDAQ/Pro+


Because WINDAQ/Pro+ recording software has the ability to sample different channels at different rates, it calculates the sample throughput rate differently than WINDAQ/Lite or WINDAQ/Pro recording software. To calculate a total sample throughput rate for WINDAQ/Pro+ software, multiply the number of channels to record by the rate of the fastest channel. For example, suppose you want to record four channels of data, one at 2kHz and the other three at 20Hz. The sample throughput rate in this case would be 8kHz (4 channels × 2kHz = 8kHz).

# Step 4 Specifying Gain and Measurement Range

Note: Some Products do not support this feature.


Choose a gain factor (varies by instrument) to get the best possible measurement resolution for your signals. A gain of 1 (unity) provides the widest measurement range possible on any given instru-





If the signals you plan to record need the wide measurement range that a gain of 1 provides, then skip this step. Otherwise, continue with this step to select a higher gain factor (thus narrower measurement range) for the best possible measurement resolution.

 Click the left mouse button in the unselected channel's annotation margin to select an analog channel for gain adjustment. A box will surround the Variable Waveform Assignment Indicator of the channel selected. The Variable Waveform Assignment Indicator displays the window number and the channel assigned to that window (X=Y: X=window number; Y=channel number).

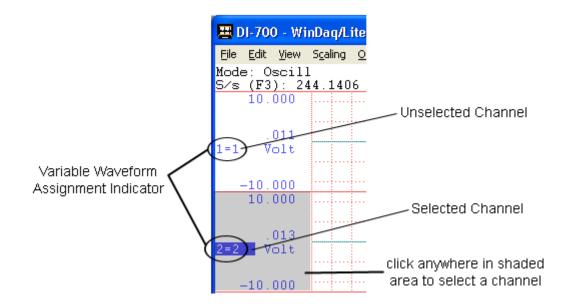



- Channel 1 Settings -FS Volt +FS Volt Acquisition Method Gain 1 -10.00010.000 Average 10 -1.00001.0000 100 .10000 -.10000 Last Point 1000 -.010000.010000 Maximum Minimum <u>R</u>MS C Frequency Input Type Einear O Nonlinear O Thermocouple Unipolar Fahrenheit 0K Cancel Reset Cal. Previous Next
- 2. Click on **Channel Settings...** in the **Edit** menu. This displays the Channel Settings dialog box:

The Channel Settings dialog box displays the hardware-dependent gain factors and equivalent plus and minus full scale voltages that result from selecting that gain factor—voltages vary by hardware device.

- 3. Click on the desired gain factor.
- 4. Click OK or press the ENTER key.


Plus/Minus full-scale annotation adjusts to reflect the application of various gain factors. You cannot adjust gain factor while in RECORD mode. See the Channel Settings Function in the Help File for complete details regarding channel settings.

## Step 5 Converting Volts to Engineering Units

EU Settings allows you to view and record waveform data in significant engineering units—converting measurements from volts to a more meaningful unit of measure. WINDAQ can scale, annotate, and display data in PSI, RPM, lbs, ft/s, or whatever engineering unit you specify.



 Click the left mouse button in the unselected channel's annotation margin to select an analog channel for gain adjustment. A box will surround the Variable Waveform Assignment Indicator of the channel selected. The Variable Waveform Assignment Indicator displays the window number and the channel assigned to that window (X=Y: X=window number; Y=channel number).

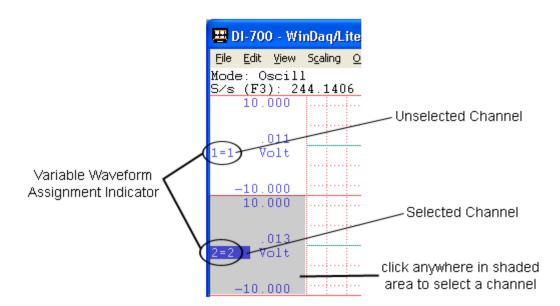

2. Click on Engineering Unit Settings... in the Edit menu.

Channel 1 Engineering L	Init Settings		X
Vol	ts E	U EU	Tag 🛛 👔
Upper Level 🗾 10.0	00 = 10.0	00 Voli	1
Lower Level 💉 .000	= .000		
Previous OK	Next	Set Offset	Cancel

3. When the relationship of volts to engineering units is known, define the relationship in the provided text boxes. For example, you know 5V equals 1500 PSI and 0V equals 0 PSI using your sensor. Enter the **Volts** and **EU** values in the appropriate text boxes as shown:

Channel 1 Enginee	ring Unit Se	ttings			×
	Volts	EL	J	EU Tag	0
Upper Level 📝	5	= 1500		DOL	
Lower Level 📝	.000	= .000		PSI	
Previous	ок	Next	Set Off	set Canc	el

4. Use the **eyedroppers** when you do not know the relationship of volts output from the sensor versus engineering units. Click either eyedropper to take a sample of the data in volts when a known engineering unit value is applied to the signal input (or found at the cursor position when using WinDaq Playback Software) for that channel. The sample value will appear in the **Volts** text box. Enter the corresponding engineering units in the **EU** text

box. Perform the same operation on the opposite end of the range. It is best to sample as close as possible to the upper and lower limits of your intended measurements to ensure accurate readings.

5. Click OK to save the settings. Note that screen scaling for the adjusted channel may change but can be redefined by selecting LIMITS... from the SCALING pull-down menu. Click Next to save the settings and open the dialog box for the next channel. Click Previous to save the settings and open the dialog box for the previous channel. Cancel exits the box without saving any settings.

You can revert to the previous EU settings at any time by using the **Reset EU** command in the **Edit** menu. Use the Set Offset button to offset the waveform (refer to the help files for more information).

## Step 6 Recording Waveforms to Disk


The Record function on the File menu initiates recording to disk. To begin waveform recording:




1. Click on **Record** in the **File** menu or press F4. This displays the Open File dialog box. Specify Click icon for Demo a file name to create a new file or open an existing file to append to it. To create a new file you must specify a maximum file size. To append an existing file you must specify how much additional data to add to it. In either case, you can specify file size in kilobytes or recording time (where sample rate determines the file size). Experiment with different file sizes, sample rates, and recording time to get the desired result. Entering information into the File Size box and pressing the TAB key will display the corresponding Recording Time in the Recording Time box and vice versa.

File Size	
File <u>S</u> ize in KiloBytes = 7	20
At a sample rate of 240 S/s, Recording <u>T</u> ime in [hours:min:]sec = 0	:25:34
ОК	Cancel


- 2. Enter the desired file size or accept the default.
- Click OK or press the Enter key to close the dialog box and begin recording to disk. WINDAQ enters RECORD
  mode and simultaneously digitizes, displays on your monitor, and streams analog channel data to disk. The Status: field in the bottom annotation line indicates RECORD.

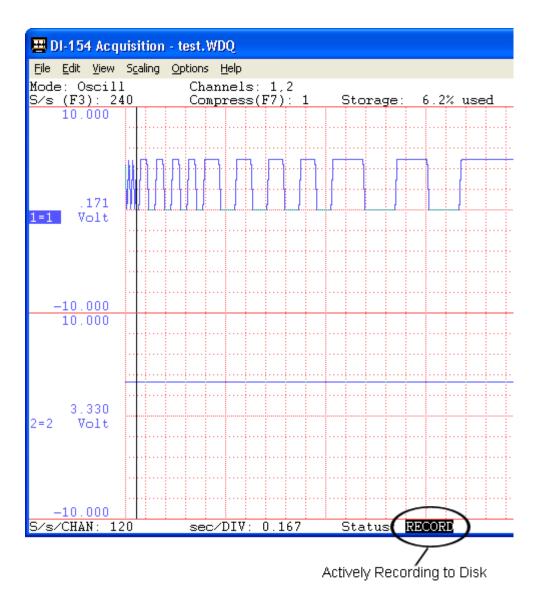


Click on **Stop** in the **File** menu or press Control + F4 to pause recording. This suspends data storage to disk, but the real time display remains active. The Status: field in the bottom annotation line indicates STBY.

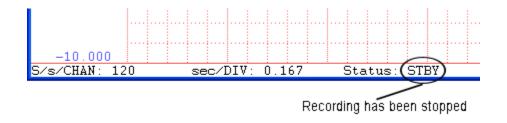

The "Storage:" field of the status bar displays the amount of file space consumed as a percentage of total file space consumed.

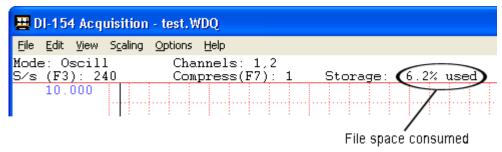

You may start and stop recording as many times as desired. When the target data file has filled, data acquisition to disk will cease, the "Storage:" field of the status bar will display "100% used" and the Status: field of the status bar will display FILE FULL.

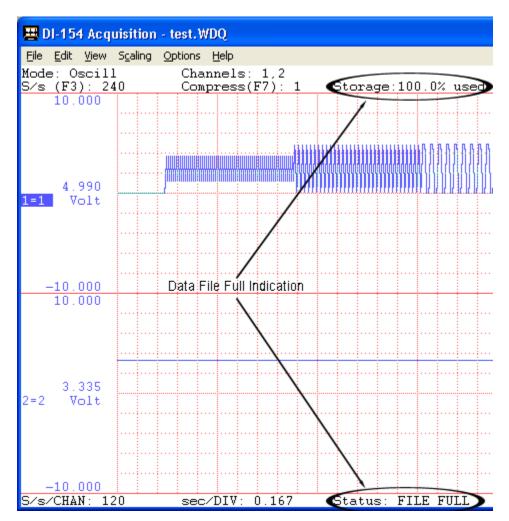

Each time recording is activated, WINDAQ inserts an event marker into the data stream. This creates acquisition break points viewable in WINDAQ Waveform Browser Playback Software and also functions as a time and date stamp.

# Additional Data Acquisition Features

Some products do not support these features—see the help files for complete details. WINDAQ Data Acquisition Software offers these functions and much, much more.

## **Event Markers**

Event Markers with comments allow you to add time and date stamped comments to the file while recording. Use event markers to mark an event or flag an uncommon occurrence in the data stream going to disk—providing a complete record of what happened and why. You automatically insert event markers in the data stream each time you activate the RECORD operating mode. These event markers get tagged with a time and date stamp that allows correlation with any point in a recorded waveform file and a precise date and time of occurrence (to the nearest second). After the data acquisition session, WINDAQ Waveform Browser Playback Software allows you to automatically search and move to the point in the data file where the event markers were placed during data acquisition (refer to the Search-For-Event function of the WINDAQ Waveform Browser Help File for more details). Refer to the Event Marker Function in the Acquisition Help Files for more information.

# Triggered Sweep Display

Triggered Sweep Display allows you to trigger the real time display so that periodic waveforms appear stationary. Set trigger conditions (such as channel, level, and slope) that define the starting point for displaying the waveform onscreen. WINDAQ displays the waveform only when data meets the trigger conditions, producing a stable display easily measured or compared to other waveforms since it starts at the same point on the screen with every sweep. The single sweep remains on the screen until waveform data again meets trigger conditions. See Display Mode Selection in the Help Files for more information.

# Triggered Mode (as supported by your hardware)

Set trigger conditions for recording data to disk. The number of pre and post trigger data points allows the user to frame an event to determine cause and effect. Set hysteresis for more reliable triggering on noisy signals. The trigger point can also be "stamped" with a vertical line in the data file. See Acquisition Triggering in the Help Files for more information.

# **Reference Files**

Reference Files allow you to define an unlimited number of default states. Specify any data acquisition file as the "set up" for a new file. All data acquisition parameters (including number of channels, channel type, scaling constants, engineering units, display format, compression, display mode, gain, etc.) from the previously recorded file become the parameters for the new data file. See Open Reference File in the Help Files for more information.

# User Annotation

User Annotation allows you to display a label (up to 30 characters) for each displayed channel. The label "rides" with the channel data and WINDAQ writes the annotation to the data file along with the acquired waveform. See User Channel Annotation in the Help Files for more information.

# 4. WINDAQ Waveform Browser

WINDAQ Waveform Browser (WWB) interprets and analyzes data during or after acquisition to disk. Make timing and amplitude measurements, review event markers, overlap waveforms to examine interdependencies, cut and paste portions of the waveform for export, and do all forms of interpretive analysis.

Follow the basic steps presented in this Chapter for a fast start to your first waveform playback and analysis session. These fast start steps outline the condensed procedure for reviewing waveforms. You will perform most of these functions every time you review data with WINDAQ Waveform Browser.

To run WINDAQ Waveform Browser software, click or double-click the WWB icon or select "Browse" in the File menu of the Acquisition software. Data acquisition does not need to be stopped to open and view the contents of a WINDAQ file. This allows interpretive analysis and measurement calculations while simultaneously recording data.

# Help Files

For a complete description of all software functions, see the context-sensitive Help Files. To access the context sensitive help either highlight a menu item and press F1 (this will take you directly to help regarding that menu item) or go to the Help menu and click on Contents. The Help Files elaborate and detail the functions in this Chapter and contain detailed descriptions of each additional function available in the WINDAQ Waveform Browser software. After you have become familiar with the functions described here, take some time to look over the rest of the functions detailed in the Help Files.


# Fast Start

# Step 1 Moving Around in the Data File

### Moving Coarsely Through the Data File with the Scroll Bar



WINDAQ Waveform Browser software allows for smooth scrolling (panning) or paging of waveforms in either a right-to-left (positive time) or left-to-right (negative time) direction. The horizontal scroll bar at the bottom of the WINDAQ window controls waveform scrolling. With it, you can move from one part of the waveform file to another. For optimum scrolling speed, position the WINDAQ Waveform Browser window entirely on the screen.



The horizontal scroll bar has the following functions:

- Click the left or right scroll arrow to scroll through the waveform 16 pixels at a time. Click and hold either scroll arrow to continue scrolling to the beginning or end of the file.
- Click anywhere in the horizontal scroll bar on either side of the slider box to scroll the waveform one screenwidth toward the beginning or end of the data file. Hold down the left mouse button to scroll rapidly until the slider box reaches the mouse pointer.

### Moving to a Single Point Using the Cursor

Click in the bottom annotation line to move the cursor directly above the point clicked. Click and drag in the bottom annotation line to allow the user to move the cursor to any single point on the screen.




You may also navigate using left and right arrow keys (if using the number key pad be sure num lock is off).

**Note:** Using a floppy disk based data file as opposed to a hard disk based file will adversely affect the maximum speed of waveform travel in either direction. To achieve maximum waveform scroll speed for your particular computer, copy the file to your hard drive.

## Step 2 Time and Date Display

View the Time and Date Display on the right-hand side of the bottom annotation line.




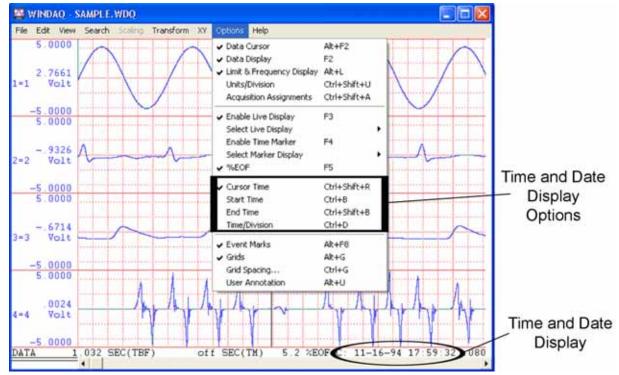

Toggle the display between Start Time, End Time, Cursor Time, and Time/Division in the Options menu.


### Start Time

The Start Time displays the date and time the file was opened for acquisition. Click on **Start Time** in the **Options** menu. An "S" displays prior to the Start Time.



### End Time


The End Time displays the date and time the file was closed for acquisition. Click on **End Time** in the **Options** menu. An "E" displays prior to the End Time.



End Time Enabled

#### **Cursor Time**

The Cursor Time displays the date and time at the current cursor position. Click on **Cursor Time** in the **Options** menu. A "C" displays prior to the Cursor Time.



#### Time/Division

The Time/Division displays the time per screen grid division. Click on **Time/Division** in the **Options** menu. A "T" displays prior to the Time/Division.


-5.0	000	and share a second state and			1
-5.0 DATA	5 684 SEC(TBF)	off SEC(TM)	28.4 %EC T:	.080 SEC/DIV	
				7	

Time/Division Enabled

### Step 3 Making Waveform Measurements with the Cursor


#### Selecting a Channel

Select a channel in WINDAQ Waveform Browser just as you would in the WINDAQ Acquisition Click icon for Demo Software i.e, click in the desired channel's left/right annotation margin. A box will surround the Variable Waveform Assignment Indicator of the selected channel. The Variable Waveform Assignment Indicator displays the window number and the channel assigned to that window (X=Y: X=window number; Y=channel number).

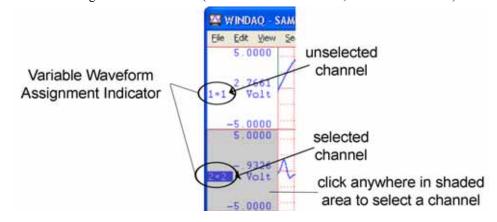


### The Data Cursor

The Data Cursor allows annotation of waveform values at the point of waveform/cursor, or waveform/base line intersection. These values appear in the left/right annotation margin next to the Variable Waveform Assignment indicator. Enable the data display waveform annotation option before toggling waveform/cursor or waveform/base line values. With the data display option enabled, click on **Data Cursor** in the **Options** menu. A check mark next to Data Cursor indicates enabled status. Click anywhere in the bottom annotation line to activate the data cursor. Click directly under the data cursor in the bottom annotation line to disable it and enable waveform/base line intersection point values. As the following illustration shows, when cursor oriented waveform data is enabled, the cursor mode designator at the bottom of the screen indicates DATA. When base line oriented waveform data is enabled, the cursor mode designator indicates BASE.

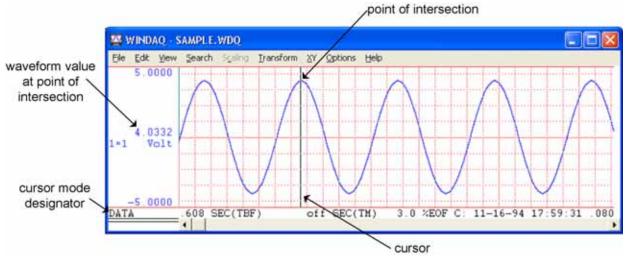

The annotated waveform value outputs either the raw waveform voltage or the waveform voltage converted into engineering units (if calibrated).

When in BASE mode use the Page Up and Page Down keys to change the baseline value of a selected channel. This shifts the waveform up or down on the screen. The upper and lower chart edge values change to center the baseline value.

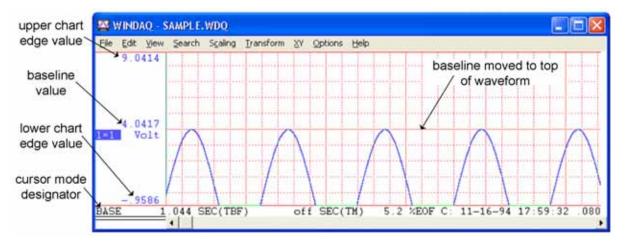

The baseline value outputs either the raw waveform voltage or the waveform voltage converted into engineering units if calibrated.

### Moving the Cursor to the highest peak

Select a channel in which to find the highest point. Click on **Peak on Screen** in the **Search** menu or double click the left mouse button anywhere in the bottom annotation line. This moves the cursor to the highest waveform peak displayed on the screen for the selected channel.

#### Moving the Cursor to the lowest valley

Select a channel in which to find the lowest point. Click on **Valley on Screen** in the **Search** menu or double click the right mouse button anywhere in the bottom annotation line. This moves the cursor to the lowest waveform valley displayed on the screen for the selected channel.

### Moving the Cursor to the Center of the Screen

Click on **Center Cursor** in the **Search** menu or click the right mouse button in the bottom annotation line. This moves the cursor to the enter of the screen. If your computer's Scroll Lock function is enabled, the waveform will move to the center of the screen along with the cursor.

# Step 4 Getting a Bird's Eye View of All the Data or a Portion of the Data

WINDAQ allows compression of data to display a whole file on-screen or display portions of data in one screen-width. Click on **Compression...** in the **Edit** menu to access waveform compression options. This displays the waveform compression dialog box.



Compression			
Compressio	CALLER CONTRACTOR		
Compresse	d Data Display:	C MAX	⊂ M×Mn
ОК	1 1	Maximum	Cancel

### **Compressing all Data**

To compress an entire file into one window-width click on the Maximum button in the compression dialog box. To fully uncompress the file click on the 1 button in the compression dialog box. The cursor position in maximum compressed mode will become the center of the screen whenever lowering compression.

### **Compressing to a Ratio**

The selected waveform compression ratio outputs in the Compression= text box. The Compression ratio equals the number of data points evaluated for a min/max value for each enabled channel. For example, if the compression ratio equals twenty, then twenty data points are evaluated to plot a min/max point. This ratio can range from -10 to whatever value required to compress the entire file on the screen (Maximum). Entering negative values in the Compression text box will expand the waveform. To find the maximum possible compression value: Fully compress the waveform (Maximum); then re-access the compression dialog box (Edit > Compression...)—the Compression= text box displays the maximum possible compression value. To increase or decrease the compression ratio enter the desired number. If you choose a compression value that is too large, an "Invalid Compression" message box will appear. Click OK or press ENTER to clear the message box and try a smaller compression value.

### Cursor Mode Control (Mid/Min/Max/MxMn) for compressed displays

The waveform compression function operates by accumulating x number of waveform samples (where x equals the compression ratio). WINDAQ calculates these values and displays a min/max line where the end points of the line equal the absolute minimum and maximum values detected for the sample group. The cursor mode control allows you to specify the desired value to report as either the minimum (MIN), maximum (MAX), mid point (MID), or maximum and minimum values (MxMn). To select the desired line segment reporting method click the desired option button and click OK.


The currently active cursor mode displays at the bottom of the screen where the DATA annotation is replaced by MIN, MAX, MID, or MxMn (default = MID). Both maximum and minimum values (separated by a slash, in the left/ right annotation margin) are displayed in MxMn mode.

# Step 5 Making Statistics Measurements

Extract and save statistics in text format for a specified section of any single waveform or for all waveforms in a file. This is a quick and easy way to get just the data desired rather than looking at all the numbers from a complete file.



- 1. Select a channel by clicking in the desired channel's left/right annotation margin. If you did not select a channel, the Open Statistics File dialog box will open allowing you to save the statistics for all channels in a spreadsheet or text format.
- 2. Position the cursor at the beginning of the desired range.
- 3. Press F4 or select Enable Time Marker in the Options menu to enable the time marker. This will place a check mark next to Enable Time Marker in the Options menu and will also show an increment of time in the bottom annotation line by the Time Marker (TM). When initially enabled it will show ".00 SEC(TM)." When disabled it will read "off SEC(TM)." The Time marker display format may be changed by selecting Select Marker Display in the Options menu.

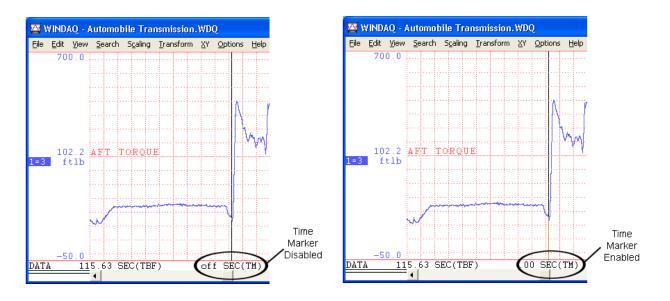

4. Position the cursor at the end of the desired range. Click on Statistics in the View menu. If a channel has not been selected, the Open Statistics File dialog box will open allowing you to save all statistics for all channels to a text or spreadsheet file. If a channel has been selected, the Statistics window opens.

UNITS	"AMPS"	
CHANNEL #	2	
# OF POINTS	334	
MEAN	1.3921E 03	
STD DEVIATION	6.2041E 02	
MINIMUM	2.1057E 02	
MEDIAN	1.2428E 03	
MAXIMUM	3.0972E 03	
RMS	1.5237E 03	
SUM	4.6496E 05	
SUM OF SQUARES	7.7545E 08	
VARIANCE	3.8491E 05	
SKEWNESS	7.2185E-01	
SLOPE	5.6651E 01	
AREA	3.0999E 04	
START POINT TBF	16.53	
END POINT TBF	38.74	
FILE	DC Drive Systems 3.V	VDQ
Write to File	Open New File	To Clipboard
TTTTL WITHER		To cubooard
Next	Previous	Cancel

The Statistics window will display the statistics for the currently selected channel including significant engineering units, channel number, the number of samples the statistics are derived from, and the file name, as well as the mean, deviation, minimum, slope, area, and position in the file. Use the Next and Previous buttons to view other channels in the file. Statistics will work with any level of compression—even fully compressed.

The To Clipboard button allows the user to save the current statistics window to the Windows clipboard. This data can then be "pasted" (CTRL + v) into a file. The Open New File... button will save data to file (if you select a channel it will save only that channel—if you do not select a channel it will save ALL channels' data). Save data in spread-sheet format (with comma delimiters) or text format. The Write to File... button allows you append an existing file.


## Step 6 Exporting to Excel

Use the **Save As...** command in the **File** menu to export a user-specified range of data from an existing data file to an Excel file.




1. Select the copy range (all data for each channel lying between the time marker and the cursor):

a. Position the cursor at the beginning of the desired range.

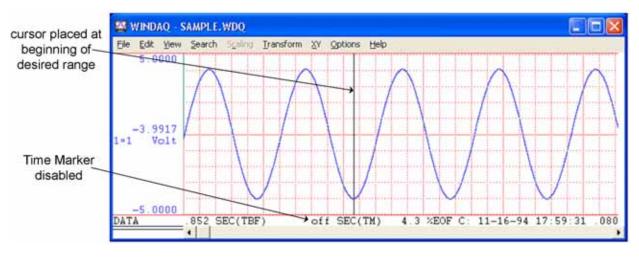

- b. Press F4 or select Enable Time Marker in the Options menu to enable the time marker. This will place a check mark next to Enable Time Marker in the Options menu and will also show an increment of time in the bottom annotation line by the Time Marker (TM). When initially enabled it will show ".00 SEC(TM)." When disabled it will read "off SEC(TM)." The Time marker display format may be changed by selecting Select Marker Display in the Options menu.
- c. Position the cursor at the end of the desired range. *Note:* Shading shown below is for demonstration purposes only. Shading does not appear in WINDAQ Playback Software.

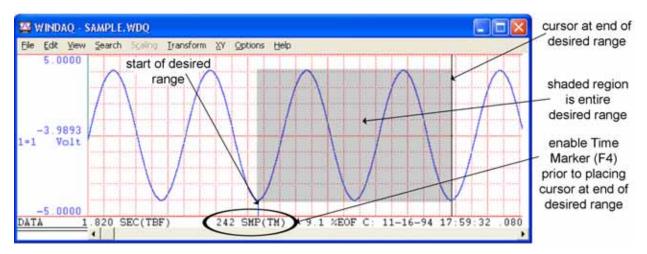

2. Click on Save As... in the File menu. This displays the Save As dialog box.

	Save As	2
pe in the csv" file ktension	File game: Itel Cov Save as type: Save As Files (".cov)	<ul> <li>Visible channels only</li> <li>Output all values when compressed</li> <li>1) ASCII (sequential)</li> <li>2) Binary (with CDDAS header)</li> <li>3) Binary (without CDDAS header)</li> <li>4) ASYST(ANT)</li> <li>5) Spreadsheet print (CSV)</li> <li>6) Deferred Hard Copy</li> <li>7) DADISP</li> <li>8) CALC</li> <li>9) EASYEST LX or AG</li> <li>A) inSoft DAC</li> </ul>

select Visible channel only to export JUST the waveforms displayed on screen

- 3. Select the file storage format option 5) Spreadsheet print (CSV). The file storage format selections appear on the right side of the dialog box. A description of each data storage format is included in the Help Files for the WINDAQ Waveform Browser software.
- 4. Enter a file name in the File name dialog box. Include ".csv" as the file extension in the file name. For example, enter "test.csv" into the file name dialog box. Click on Save to export the data—this copies the data within your selected range and from every channel in the file to the specified data file. To save only the channels displayed on-screen select the Visible channels only box in the top right hand portion of the Save As dialog box. To export specific channels, see the Extract Channels function in the Help Files.
- 5. The Spreadsheet Comments dialog box allows you to export annotations from the WWB file and allows you to add new comments. Click in the appropriate check box to transfer Sample Rate, Comments, User Annotation, Engineering Units, Relative Time, or Event Marks. After selecting the desired options and adding comments, click the OK button to close the dialog box and save the file.

Spreadsheet Comments					
Samples per sec. = 25					
Spreadsheet Comment	[]=				
test1					
Spreadsheet Comment	2 =				
Sample Rate	✓ Comments	Vser Annotation			
Engineering Units	🗆 Relative Time	Channel Event Marks			
OK		Cancel			


6. The file will have an Excel icon—double-click on the file to open it in Excel.




7. Convert data from scientific notation by changing the format of the cells to "Number" format. Highlight the data, in the **Format** menu click on **Cells...** then choose the desired format.

EL M	icrosoft Excel - test									
180	Bie Edit Yew Insert I	Format Iooks Data	Window !	jelp A	Sobe PC	Æ				
D		af celena	Ctri+1	Σ /	21	1 2				
100	10 N	Bow	•							
1.0000	At •	Çolumn	1							
	A	Sheet		D		E				
1	Samples per sec. = :	AutoFormat								
	lest1	Conditional Forma	itting	_	_		_			
3	8 MA	*		-	-		-			
the second se	Sine Wave -			-	-		-			
5	Volt -3.991		_		-		-			
7	-3.96				-		-			
8	-3.938		Format C	olle					6	×
9	-3.90	E+00	nonmar e							
10	-3.861	Contraction of the second seco	Number	Alignm	ent	Fork	Border	Patterns	Protection	
11	-3.811		Category			Samp	6			
12	-3.751	the second se	General			Samp	iles per se	$c_1 \approx 250/1$		
13	-3.68		Currency		-21	Decima	l places:	2	-	
15	-3.518	C10000	Accounts	ng l			Services.	-		
16	-3.411		Date			TUN	1000 Sec	parator (.)		
17	-3.311		Percenta Fraction	ge			ve number			
18	-3.208	E+00	Scientific			+1234	10		1	
19	-3.078		Text Special			1234			1	
20	-2.93	C1000	Custom		-1	(1234			*	
21	-2.78									
22	-2.63	COLUMN D	the sector of the	and the		d director in	e i ander		and Accounting	
24	-2 31		offer spec						and Accounting	
25	-2.15									
26	-1.988	and the second sec								
27	-1.808									
28	-1.61	and a second sec						OK	Cancel	
29	-1.42				1		-			
30	-1.23		_		-		-			
31	-1 04	2003.00			-		-			
33		E-01			-		-			
10	-0.42	L-101								

8. Manipulate your data using any Excel function. Click on **Chart...** in the **Insert** menu to create a graphical representation of your data.

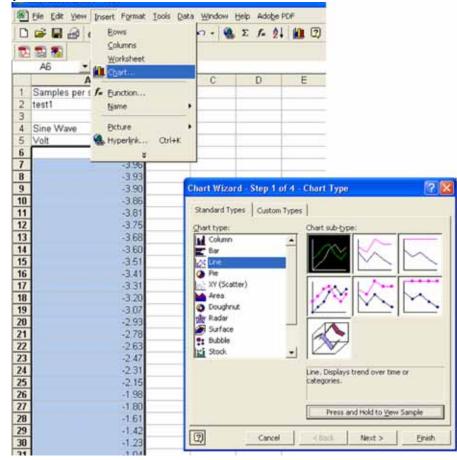

9. Choosing a Line chart will output a chart identical to the waveform exported from WINDAQ Waveform Browser.

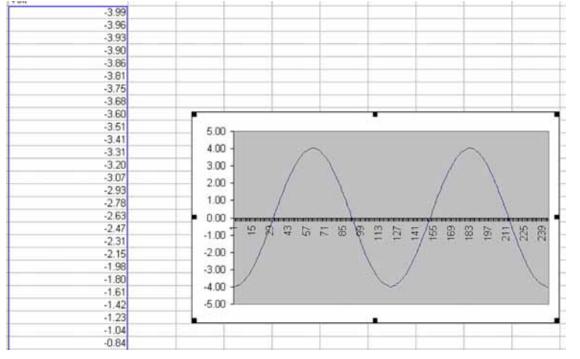

WINDAQ Waveform Browser

# Additional Playback Features

# X-Y plotting

Plot one channel versus another. Plot any two amplitude/time (Y-T) oriented waveforms versus each other - one channel designated as the X-axis and one as the Y-axis. Make analytical measurements on the X-Y plot including measure excursion, slope, and area. Static and Dynamic generation of X-Y plots are possible. See X-Y Plotting Operations in the Help Files for more information.

# FFT and DFT utilities

Perform waveform frequency analysis functions using Fourier Transform Operations. The Fast Fourier Transform (FFT) method is ideally suited for waveforms having a similar cyclic repetition. Use the Discrete Fourier Transform operation to select a portion of the waveform more accurately than the FFT. See Fourier Transform Operations in the Help Files for more information.

# **Event Markers**

Display the list of event markers and comments enabled during acquisition. Automatically locate event markers enabled during acquisition, display the date and time at the cursor position, quickly vector to any part of the data file, and enable or disable event marker display. Edit, delete, and add Event Markers in the data file. See Event Mark Editing and Search-For-Event in the Help Files for more information.

WINDAQ Waveform Browser offers these features and much, much more.

# 5. ActiveX Controls

Active X Controls eliminate lines of code from your program by having an already-made, tested, and defined function. Combine multiple ActiveX controls to perform a multitude of functions. In fact, you can combine Active X controls from any combination of vendors. Refer to numerous lines of code that have already been tested and are ready to go to work for you in just one line of code.

ActiveX controls have three types of functions: properties, methods and events. Properties are the attributes of the control. They describe the appearance and operation of the control. Methods are function calls inside the control that allow information about the control to be sent or received. Events are notifications generated by a control in response to some particular occurrence.

DATAQ ActiveX Controls support the following products: DI-148U, DI-150, DI-151, DI-154RS, DI-158 Series, DI-190, DI-194RS, DI-195B, DI-4xx products, DI-5xx products, DI-7xx products, DI-5001.

# Help Files

For a complete description of all properties, methods, and events, see the context-sensitive Help Files. To access the context sensitive help select a control or a specific property, method, or event, and press F1 (this will take you directly to help regarding that control, property, method, or event). The Help Files elaborate and detail each property, method, and event and provide sample program coding to help get you started.

# Accessing ActiveX Controls


ActiveX controls are installed when WINDAQ is installed and can be accessed in any application that supports them. For example, it takes two steps to start using ActiveX controls in Visual Basic:

- 1. Right click on the tool bar and select "Components" from the pop-up menu. This opens the Components Window.
- 2. Check the boxes in front of the five DATAQ Instruments components (DataqFile, DataqSdk, DataqSerial, DQChart, and WinDaq). Then click "OK."



omp	onents	
Con	trols Designers Insertable Objects	
	AxBrowse AxCtrl32 OLE Control module bpcctl 1.0 Type Library br549 OLE Control module C:\WINDOWS\SYSTEM\TDC.OCX Cdlg	1
	CSSEdP d2hframe 1.0 Type Library DATAQ Instruments DataqFile Control DATAQ Instruments DataqSdk Control DATAQ Instruments DataqSerial Control DATAQ Instruments DQChart Control DATAQ Instruments WinDaq Control	v
4		•

You will see the ActiveX control symbols on your tool bar.

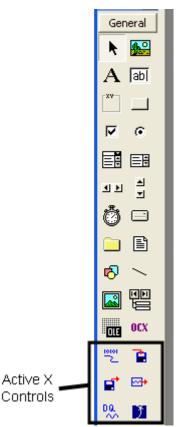

Double-click on the symbol to apply one to your form. To access the help files, select the control or select a specific property, method or event and press the F1 key.

# DataqFile

DataqFile is comprised of two components: WriteDataqFile and ReadDataqFile.

WriteDataqFile

🖹 WriteDataqFile Control

Use WriteDataqFile to create WINDAQ-compatible files. This control ensures that the files created by your program may be used with WINDAQ Waveform Browser software.

Features of WriteDataqFile include:

- File manipulation utilities that allow controlled access to data.
- +/- Full-scale definitions per channel in engineering units.
- Sample rate throughput definition that is used by WINDAQ browser software for timing measurements.

WriteDataqFile has the following limitations:

- Supports only regular WINDAQ files (i.e., no support for different channels sampled at different rates).
- No commented-event marker support.
- No user annotation support.

# ReadDataqFile

🖬 ReadDataqFile Control

Use ReadDataqFile to read WINDAQ-compatible files. In many instances, you may wish access to data acquired by WINDAQ data acquisition software. Examples include custom analysis and export requirements. This control provides a convenient way to perform these special operations.

Features of ReadDataqFile include:

- Open and close file manipulation capability.
- File navigation utilities.

It also has the following limitations:

- Supports only regular WINDAQ files (i.e. no support for different channels sampled at different rates).
- No commented-event marker support.
- No user annotation support.

# DataqSDK



DataqSdk provides access to the most basic elements of data acquisition hardware. Use DataqSDK with all DATAQ Instruments' hardware, including the DI-148U, DI-150, DI-151, DI-154RS, DI-158 Series, DI-190, DI-194RS, DI-195B, DI-4xx products, DI-5xx products, DI-7xx products, DI-5001.

Features of DataqSDK include:

- Data acquisition mode definitions for continuous and triggered data acquisition.
- Sample rate, channel, single-ended and differential definitions and various other scan list items.
- Immediate mode access to digital I/O and analog outputs.
- Access to acquired data using either burst or streaming methods.
- And more.

Limitations include:

• DataqSDK does not currently offer streaming DAC output.

# DataqSerial (Obsolete)

💆 DataqSerial Control 🛛

*Note:* The DataqSerial control is now obsolete and will no longer be supported. The DataqSDK control should now be used with serial devices. Some serial port devices may not work with DataqSerial.

Use DataqSerial with all DATAQ Instruments' hardware that supports a serial (COM port) interface, including the DI-150/151/190/194/195 series devices. Use the DataqSDK control to access and manipulate all other DATAQ Instruments' hardware products like the DI-22x/4xx/5xx/7xx series devices.

DataqSerial features include:

- Continuous access to acquire data.
- Sample rate, COM port and acquired channel definitions.
- Access to acquired data using streaming methods.


# DQChart

DQChart provides basic charting capabilities (as demonstrated in the Visual Basic samples included in the ActiveX installation).

DQChart features include:

- Plots up to 16 channels on the same chart.
- Allows analog or digital plotting.
- Displays color legends at the upper left corner of the chart.
- Supports scaling and offsetting via mouse control.
- Supports WINDAQ compatible event marker.
- Plots a specified channel from a data stream.

# WinDaq



Use the WinDaq control to eavesdrop on the data stream being acquired by WINDAQ Data Acquisition software. Use this control to return a single value or the latest frame of data (using the data frame methods) or monitor the whole data stream (using the data stream methods).

The primary advantage of this control is to relieve you of the tasks associated with initializing data acquisition. These include, but are not limited to, scan list initialization and management, sample rate definitions, engineering unit scaling and many others. These tasks are performed by WINDAQ turnkey data acquisition software at a very high level. However, the data acquired by the application can be made available in real time by this control. In this manner, the control allows you to concentrate on specific requirements of the task at hand without regard to mundane and obscure data acquisition details.

WinDaq offers the following features:

- Derives the number of channels, sample rate, engineering units scaling, m and b scaling constants and fullscale ranges in engineering units as defined by Windaq software for each channel.
- Provides access to acquired channel data using one of three options: immediate mode by defined channel, immediate mode by all enabled channels and a stream approach that guarantees waveform continuity.
- Allows asynchronous access to the hardware's digital input and output ports and analog output ports.

# 6. XControls Software Option

DATAQ Instruments and Iocomp Software have collaborated to create XControls, a collection of software modules that allow programmers and non-programmers alike to produce stunning graphical user interfaces (GUIs) for their data acquisition applications. Designed specifically for DATAQ Instruments customers, the XControls work seam-lessly with WINDAQ software. The "Linked Cell" property of each control provides exceptional power when coupled with WINDAQ/XL software. WINDAQ/XL allows WINDAQ-acquired data to be ported to definable Excel cells both in real time and after acquisition from the WINDAQ Waveform Browser (available on the DATAQ Instruments web site). When those cells are linked to any given XControl using its LinkedCell property, the control has real-time access to data: Thermometer columns rise and fall, panel meter displays update, angular display needles rotate to values, and LED bar graphs change color and size. This is just one example of the many features included in the XControls.

# Installing XControl Software

- 1. Insert the Iocomp CD-ROM into your CD-ROM drive. The installation should start automatically if you have the AutoRun option turned ON. If it does not, open "My Computer" and then double-click on your CD-ROM drive.
- 2. Click on "Install Iocomp Components Version 2.0."
- 3. Choose the folder where you want the files saved. Click Next.
- 4. When the "Welcome" window opens, click Next again.
- 5. Read the Terms of License Agreement. If you accept these terms, click Next.
- 6. Enter your user name and company name. Press Next.
- 7. Reconfirm the destination folder you selected in step 3. If correct, click Next. If incorrect, press "Browse" and locate the correct folder.
- 8. Select "Typical Setup" to install all appropriate files required for your product and for the development environments automatically detected on your computer system.
- 9. In the Keycode Manager Window, enter your keycode in the "New Keycode" text box on the right. Your keycode can be found on the label on the outside of the CD case. Please keep this number in a safe place as you will need it for future installations and updates. Once you have entered your keycode, press the "Add Keycode" button below the text box and then press Next.
- 10. In the next window, select the Development Environments that you wish to support. Auto-detected Development Environments have already been selected. Add any others you wish to support and press Next.
- 11. In the OPC Options and Settings Window, choose whether or not you want to install support for OPC features. Then press Next.
- 12. The Install Shield Wizard Complete Window will come up next. Choose if you would like to register your product (Internet access is required) or display the Instrumentation Components Directory. Then click Finish.

# Using XControls with WINDAQ/XL

This tutorial will show you how to use XControls in Excel with WINDAQ/XL. WINDAQ/XL is DATAQ's software add-on to WINDAQ Software that allows data acquired by these packages to be ported to a Microsoft Excel spread-

sheet. Let's say you need to measure the power and endurance of a motorcycle engine. You may want to test the engine to see how long it can run at its maximum level without overheating. This would involve a control to measure RPM, a control to measure the temperature, an odometer control, and an LED control that will let you know immediately when the engine has overheated. When you place all of these controls on a panel and label them, it might look something like this:



Create and link controls in Excel in four simple steps:

#### Step One:

Go to View > Toolbars > Control Toolbox. This will display the Control Toolbox. Click on the "More Controls" but-

ton 🔭 in the lower right corner to reveal additional controls.



# Step Two:

XControls have an "i" in front of them. When you find the one you want, click on it once. Your cursor will become a cross hair. Click and drag to size the control or just click where you want it to be placed on the screen and it will appear at its default size. In the example below, the iThermometer control was placed at its default size.

distant.								
	Eile Edit View Insert Format Tools Data Window Help							
	🖻 🔒 🔮	9 🖪 ×	) - Σ   C	2) 🙄 🖓 🕄	"  B   🗐	<u> </u>	? 📩 🖓	Prompt 🍟
i	iKnobX1 = =EMBED("isAnalogLibrary.iKnobX","")							
	A	В	С	D	E	F	G	
1		Volt	Volt	Volt				
2	5.737305	4.272461	1.953125	-11.8408	WinDa	q-XL	×	
3	5.737305	4.272461	1.953125	-11.8408		<b>.</b> 110 <b>E</b>		
4	5.737305	4.272461	1.953125	-11.8408			. g.	
5	5.737305	4.272461	1.953125	-11.8408				
6	5.737305	4.272461	1.953125	-11.8408	- Contr	ol Toolbox	×	
7	5.737305	4.272461	1.953125	-11.8408	🔛 🖻			
8	5.737305	4.272461	1.953125	-11.8408		Q <b>P</b>		
9	5.737305	4.272461	1.953125	-11.8408	🔽 🖬			
10	5.737305	4.272461	1.953125	-11.8408				
11	5.737305	4.272461	1.953125	-11.8408			⊠  <u>∿"</u>	
12	5.737305	4.272461	1.953125	-11.8408				
13	5.737305	4.272461	1.953125	-11.8408				
14	5.737305	4.272461	1.953125	-11.8408	0	• -1	00	
15	5.737305	4.272461	1.953125	-11.8408		E		
16	5.737305	4.272461	1.953125	-11.8408		E 7	5	
17	5.737305	4.272461	1.953125	-11.8408		Ξ.		
18	5.737305	4.272461	1.953125	-11.8408	0		0 0	
19	5.737305	4.272461	1.953125	-11.8408		= 2	5	
20	5.737305	4.272461	1.953125	-11.8408		E		
21	5.737305	4.272461	1.953125	-11.8408		🛛 📕 🗄 o	E	
22						•	0	
23						0	0	
24								-
44	K ( ) N Sheet1 / Sheet2 / Sheet3 /							
	Ready NUM /							

# Step Three:

When the control is placed, you will automatically enter "Design Mode." Right click on the control and select "Properties" or just press the Properties button in the Control Toolbox. Here, you can change the properties of your control, such as size, style, font, etc., but, most importantly, you can link the control to your application. Next to "LinkedCell," type in the Column and Row of the cell to which you would like the control linked. For example, to specify a cell in Column "C," Row 5, you would just type "C5."

ThermometerX1 iThern	nometerX	
Alphabetic Categorized		
(About)		
(Custom)		
(Name)	iThermometerX1	- 11
AutoCenter	True	
AutoLoad	False	
AutoScaleDesiredTicks	5	
AutoScaleEnabled	False	
AutoScaleMaxTicks	6	
AutoScaleStyle	0 - iassAutoMinMax	
BackGroundColor	8H800000F&	
BackGroundPicture	(Bitmap)	_
BorderStyle	0 + ibsNone	
CurrentMax	0	
CurrentMin	0	
Enabled	True	
EndsMargin	10	
Height	112.5	
IndicatorBackGroundColor	8H000000808k	
IndicatorBulbSize	6	
IndicatorColor	8H00000FF&	
IndicatorStyle	0 - itisBulb	
IndicatorWidth	2	
Left	237.75	
LinkedCell	CS	
Locked	True	
MaxPointerColor	8H00FFFF00&	+1

You can change other properties by right clicking on the control and selecting "(the name of your control) Control Object" and then click on "Properties" (for our example, you would select "iThermometerX Control Object" > "Properties").

	0 100			
2	- 100 - 75 - 50 - 25 - 0	0		
, ,	÷=0 0	% ©	Cut_ Gopy Paste	
		2 2	Properties View Code	
		-	Grouping	Properties
			Order +	
		39	Eormat Control	

Control About Control Design Auto Scal	· · · · · · · · · · · · · · · · · · ·	
Control Design Auto Scal		
	e OPC Theme	
Position 0 Position Max 100 Position Min 0 Current Max 0 Current Min 0	Cached Drawing Transparent	
Update Frame Rate 60	Auto Frame Rate	Apply

This displays another window specific to the control (shown below for the "iThermometer" control).

#### Step Four:

To exit Design Mode and apply any property changes you have made to the control, click the "Exit Design Mode"

button in the upper left-hand side of your Control Tool bar. This is also the button you need to press if you want to enter Design Mode at any point to make changes to the control.

Your control is now linked!

# **XControls Documentation**

The documentation for the XControls is on the CD as a pdf. To view the documentation, you must have Adobe Acrobat Reader. If you do not have Adobe Acrobat Reader, download it for free off the Internet at www.adobe.com. To access the documentation, insert the CD. Close the Installation window. Double click on "My Computer" and then right click on the CD-ROM drive. Choose the "Explore" option. This opens a window containing all of the folders on the CD. Open the "DOC" folder and then, inside that folder, open the "General" folder. Inside this folder is the "Getting Started Guide" pdf you need to use XControls.

The Getting Started Guide includes everything you need to operate XControls, except for the instructions for use with WINDAQ/XL, which is included in this manual.

Chapter One covers which component architecture you should use. ActiveX, VCL and CLX component architectures are included with your XControls. This chapter also gives an overview of XControls' key features and system requirements and tells you where you can locate help.

Chapter Two describes installation procedures, including custom setup, repair, service packs, and uninstall instructions as well as other procedures.

Chapter Three describes how to get started using the ActiveX component architecture. It covers setting up component projects within Visual Basic and Microsoft Visual C++, including modifying control properties, generating even code, basic programming usage and accessing help files. Chapter 3 also provides directions on distributing ActiveX Component Files.

Chapter Four covers how to get started using the VCL component architecture. It describes the process of compiling and installing VCL components, accessing help files, distributing components, setting an environment library path, modifying control properties, generating event code, and basic programming usage.

Chapter Five describes how to get started using the CLX component architecture. It covers setting up component projects in Borland Delphi, C++ Builder, and Kylix, including compiling and installing CLX components, accessing help files, distributing CLX components, modifying control properties, generating event code, and basic programming usage.

Chapter Six details support options for XControls.

Appendix A contains a chart detailing each component library and what components they include.

Appendix B contains a table listing commonly used colors, their hexadecimal values and selected constants from popular development environments.

Appendix C details the Transparency Feature, including how and when it can be used.

Appendix D details the Themes Feature, including how to use existing themes, how to create your own, how to use themes in a compiled application using Run-Time Property Editors and more.

Appendix E contains the Software License Agreement.

# Index

### Numerics

100% used 19

## A

accessing ActiveX Controls 33–34 acquisition software 7–20 ActiveX Controls 33–36 DataqFile 34–35 DataqSDK 35 DataqSerial 35 DQChart 36 WinDaq 36 analysis software 21–32 annotation 20 annotation margin 14, 15, 23

# B

BASE 23 baseline oriented waveform data 24 baseline value, upper chart edge value 24 bottom annotation line 23 Browse 21 browsing a data file 21-??

# С

calibrating input signals 15-?? Center Cursor 25 channel expander 8 Channel Selection grid 8 channel settings dialog box 15 Channel Settings... 15 channels differential 9 digital input 9 fixed differential 9 Channels field 7, 8 Channels... 7, 8 compressing data to a ratio 25 compressing waveform data 25 compression ratio 25 Compression... 25 context-sensitive help 1 acquisition software 7

ActiveX Controls 33 playback software 21 conventions 3 general 3 mouse 3 copy range 27 CSV 29 cursor 22 cursor mode designator 24 Cursor Time 23

# D

DATA 23 Data Cursor 23 DataqFile 34–35 ReadDatagFile 35 WriteDataqFile 34 DataqSDK 35 DatagSerial 35 date stamp 19, 20, 32 default states 20 Demonstration Video 3 **DFT 32** differences between WinDag/Lite/Pro/Pro+ Recording software 1 differential channels 9 digital input channels 9 Digital Plot 10 disabling channels other products 9 serial port products 7 display format 10 displaying channels 10-12 displaying compressed waveforms 25 DQChart 36

# E

Enable Time Marker 26, 28 enabling channels 7–10 other products 8 analog 9 differential 9 digital 9 fixed differential 9 special considerations 10 End Time 23 engineering units 15 event marker 19, 20, 32 Excel 27, 37 Cells... 30 Chart... 31 Excel icon 30 exporting waveform data to Excel 27–31 extracting statistics 25–27

#### F

F4 28 FFT 32 FILE FULL 19 file size 17 file space consumed 19 file storage format 29 fixed differential channels 9 flag 20 Format Screen 10 formatting numbers 30 fourier transform operations 32 frequency analysis 32 full scale annotation 15 full scale measurement range 14

#### G

gain 14–15 gain configuration 14 gain factor 15

#### Η

help files 1–?? acquisition software 7 ActiveX Controls 33 playback software 21 help topics 1 horizontal scroll bar 21

#### I

installing XControls 37

#### L

label 20 left/right annotation margin 23 line segment reporting 25 linking XControls to WinDaq/XL 37–41 lower chart edge value 24

#### Μ

making statistics measurements 25-27 making waveform measurements with the cursor 23-25MAX 25 maximum compression 25 measurement range 14-15 measurement resolution 14 MID 25 **MIN 25** moving around in the data file 21-?? moving the cursor to the center of the screen 25 to the highest peak 24 to the lowest valley 24 Multimedia Demonstration Videos 3 multiplexer 8 MxMn 25

#### N

negative input terminal 9 non-overlapped waveform display 11

## 0

open file dialog box 17 opening ActiveX Controls 33–34 operating mode 3–4 RECORD 4 SETUP 3 STBY 4 overlapped waveform display 11

#### P

paging through waveforms 21 pause 18 Peak on Screen 24 playback software 21–32 plotting digital data 9 positive input terminal 9

#### R

ratio, compressing data to 25 ReadDataqFile 35 RECORD 4, 17–19 Record 17–19 recording software 7–20 recording time 17 recording waveforms to disk 17–19 reference files 20 right mouse button 3 running WinDaq Waveform Browser software 21

#### S

S/s/CHAN 13 sample rate per channel 13 save as dialog box 29 Save As... 27–31 saving data to Excel 27–31 saving waveform data 17–19 scientific notation 30 scroll bar 21 selecting a channel acquisition software 14–15, 15–?? playback software 23 setting analog channels as differential 9 SETUP 3 significant engineering units 15 software license agreement iii specifying a sample rate 12–13 specifying gain and measurement range 14–15 spreadsheet comments 29 spreadsheet options 29 spreadsheet print 29 STANDBY 4 Start Time 22 statistics 25-27 statistics window 27 STBY 4, 18 Stop 18 Storage field 19

#### T

time and date display 22–23 time and date stamp 19, 20, 32 Time Marker 26 Time/Division 23 TM 26 To Clipboard 27 toggling the data cursor on/off 23 triggered sweep display 20

#### U

user annotation 20

using the cursor 22 using XControls with WinDaq/XL 37-41

# V

Valley on Screen 24 variable waveform assignment indicator 14, 15, 23 Video 3 viewing enabled channels 10–12 Visual Basic 33

#### W

waveform assignment indicator 14, 15 waveform display 11 waveform frequency analysis 32 waveform measurements 23–25 waveform value at point of intersection 24 WinDaq 36 WinDaq Software Demonstration Videos 3 WinDaq Waveform Browser 21–32 WinDaq/Lite/Pro/Pro+ differences 1 WinDaq/XL 37 WriteDataqFile 34 WWB 21–32

## Х

XControls documentation 41 XControls software option 37–42 X-Y plotting 32

#### Y

Y-Т 32